

Development and validation of ultra high performance liquid chromatographic (UHPLC) method for the determination of roxithromycin in the broiler plasma

12
13
14
15

ABSTRACT

Aims: The present study was designed to develop and validate the UHPLC method for quantitative determination of roxithromycin, a macrolide antimicrobial drug, in broiler plasma for the application of pharmacokinetic studies.

Methodology: UHPLC apparatus comprised of ultraviolet (UV) detector was used in the present study. Chromatographic separation was performed by using reverse phase C18 column. Mobile phase was combination of buffer and 55 acetonitrile in the ratio of 55: 45. Buffer part used was 0.1 % trifluoroacetic acid (v/v) having pH of 2.1. Erythromycin was used as an internal standard. Isocratic elution mode was employed with flow rate of 1 ml/min and effluents were monitored at wavelength of 220 nm. Liquid-liquid extraction using ice-cold acetonitrile was performed to extract roxithromycin from plasma samples. The data integration was performed using Chromeleon™ version 6.8 software.

Results: The linear calibration curve with a mean correlation coefficient (R^2) value of 0.9999 was observed for concentrations ranging from 0.20 to 12.80 µg/ml. At any concentration, accuracy was not found to be less than 90 %. The mean extraction recovery (n=5) for concentrations of 0.40 µg/ml was 81.36 %. The calculated intraday and interday C.V. % was not more than 7.70 % and 9.42 %, respectively, at any concentration studied. The specificity of the analysis was reflected by the narrow range of retention time ranging between 6.983 to 7.178 minutes. LOD and LOQ of the method under investigation were calculated as 0.131 and 0.398 µg/ml, respectively

Conclusion: A reliable, reproducible, accurate, precise, specific and sensitive method for analysis of roxithromycin in broiler plasma was developed and validated for application in the pharmacokinetic study of the roxithromycin.

16
17
18
19
20
21
22
23
24
25

Keywords: UHPLC, Roxithromycin, Method validation, Broiler plasma

1. INTRODUCTION

Roxithromycin is a semi-synthetic, long-acting, orally administered antibacterial drug of macrolide class [1]. One of the biggest advantages of roxithromycin is its power of intracellular concentration. The pharmacokinetic profile of roxithromycin is characterized by high plasma, tissue and body fluid concentrations and a long half-life permitting an extended dosage interval [2]. Macrolide antibiotics and their semi-synthetic derivatives like roxithromycin are most commonly used in poultry to treat avian mycoplasmosis and are considered to be bacteriostatic at low therapeutic concentrations, but can be slowly bactericidal at higher concentrations [3]. Roxithromycin is widely used as antimicrobial drug for treating many bacterial infections especially *Mycoplasma* spp. in broiler chickens. In Asian countries, its use is more in poultry industry for the treatment of Chronic Respiratory

66 **2.3 Instruments**

67

68 Ultra high performance liquid chromatography (UHPLC) apparatus (Dionex ultimate 3000[®],
69 Thermo Fisher, Germany) comprised of ultraviolet (UV) detector and gradient solvent
70 delivery pump was used in the present study. Chromatographic separation was performed
71 by using reverse phase C₁₈ column (ODS, 25 cm x 4.6 mm ID, 4.5 μ; Purospher[®] Star RP-
72 18, Merck-Millipore, Mumbai, India) at ambient temperature (~28°C). The data integration
73 was performed by software 'Chromeleon™ version 6.8' Chromatography Data System.

74

75 **2.4 Drug Extraction from Plasma Standards**

76

77 Drug-free broiler plasma was used for making different roxithromycin concentrations of 0.20,
78 0.40, 0.80, 1.60, 3.20, 6.40, and 12.80 mg/ml. After drug extraction, each of these standards
79 was run in quintuple (n=5) to get area response in UHPLC. Liquid-liquid extraction using ice-
80 cold acetonitrile was performed to extract roxithromycin from plasma samples. Exactly 400
81 μL of plasma sample was taken into 2 ml Eppendorf[®] micro-centrifuge tube, and then 40 μL
82 1 M NaOH was added to it and vortexed for about 10 seconds. After this alkalization, 1200
83 μL ice-cold acetonitrile was added in same tube and vortex mixed for 3 minutes at 2400
84 RPM. Then the mixture was centrifuged at 5000 RPM for 10 minutes at 4°C. Upper organic
85 phase was collected and dried under nitrogen (N₂) evaporator (AT-EV-50, Athena
86 Technology, Mumbai, India). Exactly, 20 μL of internal standard (200 mg/ml erythromycin
87 dissolved in diluent) was mixed with 80 μL diluent (made up of equal parts of ice-cold
88 acetonitrile and HPLC grade water) for reconstitution of each extracted and evaporated
89 sample. Thus, dried residues were reconstituted with total 100 μL diluent. The prepared
90 sample was finally centrifuged (5000 RPM, 5 minutes, 4°C) and 20 μL of the upper clear
91 portion was manually injected into UHPLC.

92

93 **2.5 Optimized Chromatographic Conditions**

94


95 The optimized chromatographic parameters for UHPLC analysis of roxithromycin
96 concentrations in broiler plasma sample are given in Table 1. Mobile phase comprises of 55
97 parts of buffer with 45 parts of acetonitrile. Buffer part was prepared by mixing trifluoroacetic
98 acid (TFA) with HPLC grade water to yield strength of 0.1 % TFA buffer (v/v) having pH of
99 2.1. It was filtered by filter paper (0.45 μm pore size) by using a vacuum pump and
100 degassed using ultrasonic sonicator before use. During sample run, intermittent washings of
101 microsyringe were done with washing solution (80 Acetonitrile: 20 HPLC grade water) to
102 avoid carry over effect.

103

104 **Table 1. Optimized chromatographic parameters for UHPLC analysis of roxithromycin**

S.N.	UHPLC parameters	Optimized values
1	Mobile phase components and ratio	55 (TFA Buffer) : 45 (Acetonitrile)
2	Elution mode	Isocratic
3	Flow rate	1.0 ml/min
4	Detection wavelength (λ_{max})	210 nm
5	Injection volume	20 μL
6	Run time	12 min
7	Retention time (RT)	7.1 min

105 The representative chromatograms are shown in Figure 2.
106

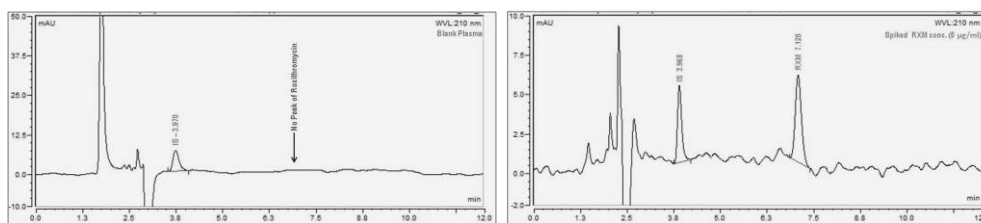

107
108

109 Fig. 2. Chromatograms of (A) blank plasma, (B) plasma spiked with roxithromycin (5 µg/ml)

110

111 UV detector responses were generated as chromatograms using 'Chromeleon™ version 6.8'
112 software at the data collection rate of 2.5 Hz and a time constant of 0.6 second.

113

114 2.6 Method Validation

115

116 For validation of the present developed UHPLC method for analysis of roxithromycin, major
117 parameters like linearity, recovery, accuracy and precision (intraday and inter-day) were
118 calculated as per standard guidelines [15, 16]. Limit of detection (LOD) and Limit of
119 quantification (LOQ) were calculated using the standard deviation of responses (Std. Dev.)
120 and the slope value of the calibration curve [17]. Formulae used were $LOD = 3.3 \times (Std. Dev. / Slope)$
121 and, $LOQ = 10 \times (Std. Dev. / Slope)$.

122

123 2.7 Statistical Analysis

124

125 All values are expressed as the mean \pm standard deviation. Precision C.V. (Co-efficient of
126 variance) was calculated as $\% = (Standard\ Deviation / Mean\ of\ observed\ concentration) \times$
127 100.

128 3. RESULTS AND DISCUSSION

129

130 3.1 Optimization of chromatographic parameters

131 The ultimate goal of optimization of any HPLC method is to achieve good resolution peaks
132 with acceptable retention times but without peak tailing, absence of the interfering
133 background peaks, and high and stable sensitivity [19]. It is easier to achieve absence of
134 interfering background peaks when analysis is to be done in simple matrices. However, for
135 the present study, involving the analysis in complex biological matrix like plasma, minimizing
136 the interfering peaks was focused. Many buffers have been used in past for reverse phased
137 chromatographic estimation of roxithromycin mainly phosphate and acetate buffers [7, 11,
138 13, 18], but in present study, trifluoroacetic acid (TFA) buffer gives good chromatographic
139 results in terms of satisfactory separation of peaks in plasma samples. It has added
140 advantage for having longer working life of silica columns. The precaution was taken to
141 prepare fresh 0.1 % TFA (v/v) each day prior to analysis due to its volatile nature. Initially,
142 gradient method was followed started with 95 % buffer and 5 % acetonitrile scheme stage
143 wise finally changed to 5 % buffer and 95 % acetonitrile at 10 minutes but was finally
144 avoided due lack of reproducibility in the terms of retention time. Finally, isocratic method
145 with 55 % TFA buffer and 45 % acetonitrile was found suitable and was adopted. HPLC
146 grade Acetonitrile (ACN) was used as organic modifier part in mobile phase as it was
147 reported to having good solute retention capacity for roxithromycin [19]. Moreover, ACN is
148 good choice when detection is to be done at lower wavelengths of 200-220 nm as it has
149 lower UV cut-off value of 190 nm. Generally, macrolides are known to show higher
150 absorbance at lower wavelengths and produce weak chromatographic signals.

151 Roxithromycin exhibits weak absorbance at higher wavelengths (235 nm) [13]. UV-detection
152 of roxithromycin has been performed at lambda max (λ_{max}) value between 200 to 220 nm [5,
153 6, 10, 13]. The three wavelengths i.e. 205, 210 and 215 were tried in the present study and
154 larger peak areas were obtained at λ_{max} of 210 nm; hence this wavelength was selected for
155 chromatographic detection of roxithromycin.

156 3.2 Method validation

157

158 3.2.1 Linearity

159

160 The linearity was tested from the calibration curve prepared from spiked plasma samples for
161 concentrations in the range from 0.20 to 12.80 $\mu\text{g/ml}$. For linearity, seven concentrations i.e.
162 0.2, 0.4, 0.8, 1.6, 3.2, 6.4 and 12.8 $\mu\text{g/ml}$ were used in quintuplet ($n = 5$) and their mean
163 values were used to construct the curve. The resultant mean linear regression equation of
164 calibration curve for roxithromycin was of $y = 0.2342x + 0.0031$ with $r^2 = 0.9999$. For the
165 individual set of values, the goodness-of-fit (r^2) was found at least 0.9987 among all five
166 curves, indicating functional linear relationship between the concentration of analyte and
167 area under the peak.

168 3.2.2 Recovery

169

170 Blood plasma is a complex mixture of biologically active compounds including proteins that
171 can bond to the target analyte or interfere with their detection. Various liquid – liquid
172 extraction (LLE) protocols with alkalization had been used to extract roxithromycin from
173 biological matrices using solvents like tert-butyl methyl ether [7], Diethyl ether with
174 isopentane [11], hexane plus isoamyl alcohol [13], dichloromethane [10] and Acetonitrile [9,
175 12]. In present study, extraction was tried with dichloromethane and acetonitrile and more
176 recovery was observed with acetonitrile. Acetonitrile is one of the most efficient organic
177 solvent which also removes protein from plasma. Ice cold acetonitrile was used to get better
178 protein precipitation. The effect of acetonitrile volume on the extraction was examined at in
179 the range of 800 to 1400 μL (2 to 3.5 times of plasma volume) and 1200 μL was found to be
180 optimal volume as the peak area of analyte was not increased beyond this volume of
181 extracting solvent. The presence of basic nitrogen(s) in macrolide molecules reflects the
182 basic character of these lipophilic compounds; pKa of roxithromycin is equal to 8.8 [12].
183 Therefore, extraction of roxithromycin from plasma needs a high pH condition (alkalization)
184 which is obtained by using 1M NaOH in the present study. Same alkalizing agent was also
185 employed in other study to get good recovery percent of roxithromycin from plasma [7].The
186 extraction recovery of roxithromycin was measured by comparison of the areas of
187 roxithromycin after injection of the extracted spiked samples ($n=5$) with those obtained after
188 injection of the standard solution containing equivalent concentrations of the drug. The
189 extraction recovery was studied at three different concentrations of 0.40 $\mu\text{g/ml}$ (low near to
190 LOQ), 3.20 $\mu\text{g/ml}$ (medium) and 12.80 $\mu\text{g/ml}$ (high concentration) as per validation
191 requirements. The respective mean recoveries were obtained in similar figures as 81.36,
192 79.83 and 81.12 % (Table 2). A higher recovery rate of roxithromycin (112 %) from rat
193 plasma was reported for amperometric detection, using tert-butyl methyl ether as extraction
194 solvent [7] whereas extraction with hexane : isoamylalcohol (98:2) exhibited $90 \pm 3\%$ recovery
195 of roxithromycin in human plasma [13].

196 Table 2: Mean extraction recoveries for roxithromycin from spiked plasma ($n=5$)

197

S.N.	Spiked Plasma Concentration ($\mu\text{g/ml}$)	Recovery (%)	Range (%)	Mean Recovery (%)
------	--	--------------	-----------	-------------------

1	0.400	75.07		
2	0.400	86.73		
3	0.400	72.71	72.71 – 94.91	81.36
4	0.400	90.93		
5	0.400	94.91		
6	3.200	70.69		
7	3.200	85.96		
8	3.200	71.46	70.69 – 92.63	79.83
9	3.200	91.23		
10	3.200	92.63		
11	12.800	72.98		
12	12.800	86.18		
13	12.800	70.80	70.80 – 94.50	81.12
14	12.800	94.50		
15	12.800	91.58		

198

199 **3.2.3 Accuracy**

200

201 Accuracy (in per cent) was estimated by deviation of observed concentration in plasma
 202 sample with spiked known drug concentration in the plasma sample. Accuracy was studied
 203 at three different concentrations in triplicates. At any concentration, accuracy was not found
 204 to be less than 90.20 % or in other terms, inaccuracy was not more than 9.8 % (Table 3). In
 205 another report [13] too, the inaccuracy did not exceed 9 % at all levels studied, which is quite
 206 acceptable.

207 **Table 3. Accuracy of the developed method for analysis of roxithromycin from broiler**
 208 **plasma (n=3)**

209

S.N.	Spiked Plasma Concentration (µg/ml)	Observed Concentration (µg/ml)	Accuracy (%)
1	0.400	0.421	97.90
2	0.400	0.446	95.40
3	0.400	0.471	92.90
4	3.200	3.127	92.70
5	3.200	3.298	90.20
6	3.200	3.116	91.60
7	12.800	12.764	96.40
8	12.800	12.889	91.10
9	12.800	12.825	97.50

210

211 **3.2.4 Precision**

212

213 Intraday and inter-day precisions (n=5) were expressed in the terms of C.V. % (Co-efficient
 214 of variance). The highest intraday and interday C.V. % calculated was 7.70 % (at 0.20 µg/ml)
 215 and 9.42 % (at 0.40 µg/ml), respectively (Table 4). Thus, it was acceptable since CV% was
 216 within the acceptable 20% limit at the lower limit of quantification (0.400 µg/ml) and within
 217 15% for other concentrations studied.

218

219 **Table 4: Intraday and inter-day precision of roxithromycin in broiler plasma (n=5) by**
 220 **UHPLC - UV detection**

S.N.	Spiked Concentration (µg/ml)	Mean Observed Area (mAU*min)	Standard Deviation	Precision C.V. (%)
Intraday values (n=5)				
1	0.200	0.0437	0.0034	7.77
2	0.400	0.1076	0.0046	4.27
3	0.800	0.1996	0.0078	3.91
4	1.600	0.3732	0.0155	4.15
5	3.200	0.7479	0.0242	3.24
6	6.400	1.4912	0.0404	2.71
7	12.800	3.0070	0.1441	4.79
Interday values (n=5)				
1	0.200	0.0497	0.0033	6.65
2	0.400	0.1147	0.0108	9.42
3	0.800	0.2152	0.0167	7.76
4	1.600	0.3918	0.0329	8.40
5	3.200	0.8457	0.0645	7.63
6	6.400	1.6702	0.1065	6.38
7	12.800	3.3259	0.2463	7.41

221

222 **3.2.5 Specificity**

223

224 This parameter is concerned with the extent to which other substances interfere with the
 225 identification and, where appropriate, quantification, of the analyte(s) of interest. The
 226 retention times of roxithromycin were specifically ranged, without any interference peaks,
 227 from 6.983 to 7.178 (~ 7.1 ± 0.1) minutes with a mean of 7.081 minutes.

228 **3.2.6 Sensitivity**

229

230 Limit of detection (LOD) and Limit of quantification (LOQ) were calculated using the standard
 231 deviation of responses and the slope value of the calibration curve. LOD and LOQ of the
 232 developed analytical method for roxithromycin were calculated as 0.131 and 0.398 µg/ml,
 233 respectively. The target quantification limit of roxithromycin in plasma for pharmacokinetic
 234 study should be above its MIC (minimum inhibitory concentration), that is 0.5 µg/ml against
 235 most of common susceptible pathogens. The MIC cut-off point for roxithromycin separating
 236 sensitive from resistant human pathogens was suggested to be 0.5 µg/ml [20] whereas, MIC
 237 breakpoints for roxithromycin against avian pathogen *Mycoplasma gallisepticum* were
 238 suggested as ≤ 1–4 (Sensitive), ≤ 4 (Intermediate) and > 4 (Resistant) µg/ml [21].

239

240 **3.2.7 Internal Standard**

241

242 Internal standard calibration involves the comparison of the instrument responses from the
 243 target compound in the sample to the responses of reference standard added to the sample
 244 or sample extract before injection [22]. The difference between retention times of the target
 245 compound and the internal standard may be used to know the relative retention time which
 246 can be further used to compensate for small retention time shifts. Roxithromycin and
 247 erythromycin were used as internal standard for quantification of each other [11, 18].
 248 Clarithromycin is also used as an internal standard in one study when pure erythromycin
 249 was not available [13]. In present analytical method for roxithromycin, erythromycin (200
 250 µg/ml concentration in diluent) was found appropriate as an internal standard, producing
 251 consistent peak area and providing wide separations between peaks of target analyte and

252 **internal standard.** Retention time of erythromycin was 4.0 ± 0.1 minutes in the present
253 method.

254

255 **4. CONCLUSION**

256

257 The developed UHPLC method for determination of roxithromycin in broiler plasma was
258 found to be reliable, reproducible, accurate, precise, specific and sensitive method, and
259 serves the purpose for the application in the pharmacokinetic study with limit of quantification
260 equal to $0.398 \mu\text{g/ml}$ which is lower than the target MIC value of roxithromycin against
261 susceptible bacterial pathogens in broiler chickens which ranges from 0.500 to $1.000 \mu\text{g/ml}$.

262

263

264 **COMPETING INTERESTS**

265

266 There is no competing interests exist.

267

268 **CONSENT**

269

270 It is not applicable.

271

272 **ETHICAL APPROVAL**

273

274 It is not applicable.

275

276 **REFERENCES**

277

- 278 1. Gaynor M, Mankin AS. Macrolide Antibiotics: Binding Site, Mechanism of Action,
279 Resistance. *Curr Top Med Chem.* 2003; 3(9):949-960.
- 280 2. Markham A, Faulds D. Roxithromycin. *Drugs.* 1994; 48(2):297-326.
- 281 3. Landoni MF, Albarellos G. The use of antimicrobial agents in broiler chickens. *Vet J.*
282 2015; 205(1):21-27.
- 283 4. Na lampang K, Chongsuvivatwong V, Kitikoon V. Pattern and determinant of antibiotics
284 used on broiler farms in Songkhla province, southern Thailand. *Trop Anim Health Prod.*
285 2007; 39(5):355-361. Available: <https://doi.org/10.1007/s11250-007-9023-3>.
- 286 5. de Oliveira V, Bergold AM, Schapoval EE. High-performance liquid chromatographic
287 determination of roxithromycin in tablets. *Anal Lett.* 1996; 29(13):2377-2382.
- 288 6. Wahba ME. Liquid chromatographic determination of roxithromycin: application to
289 stability studies. *J Chromatogr Sc.* 2012; 51(1):44-52.
- 290 7. Taninaka C, Ohtani H, Hanada E, Kotaki H, Sato H, Iga T. Determination of
291 erythromycin, clarithromycin, roxithromycin, and azithromycin in plasma by high-
292 performance liquid chromatography with amperometric detection. *J Chromatogr B*
293 *Biomed Sci Appl.* 2000; 738(2):405-411.
- 294 8. Wang P, Qi M, Jin X. Determination of roxithromycin in rat lung tissue by liquid
295 chromatography-mass spectrometry. *J Pharm Biomed Anal.* 2005; 39(3-4):618-623.
- 296 9. Torano JS, Guchelaar HJ. Quantitative determination of the macrolide antibiotics
297 erythromycin, roxithromycin, azithromycin and clarithromycin in human serum by high-
298 performance liquid chromatography using pre-column derivatization with 9-
299 fluorenylmethyloxycarbonyl chloride and fluorescence detection. *J Chromatogr B*
300 *Biomed Sci Appl.* 1998; 720(1-2):89-97.
- 301 10. Djordjevic S, Drljevic K, Jovanovic B, Kilibarda V. Determination of roxithromycin in
302 human urine by liquid chromatography with photo diode array detection. *Med Data.*
303 2011; 3(4):345-348.

- 304 11. Grgurinovich N, Matthews A. Analysis of erythromycin and roxithromycin in plasma or
305 serum by high-performance liquid chromatography using electrochemical detection. *J*
306 *Chromatogr B Biomed Sci Appl.* 1988; 433:298-304.
- 307 12. Glowka FK, Karazniewicz-Lada M. Determination of roxithromycin in human plasma by
308 HPLC with fluorescence and UV absorbance detection: application to a pharmacokinetic
309 study. *J Chromatogr B.* 2007; 852(1-2):669-673.
- 310 13. Macek J, Ptacek P, Klima J. Determination of roxithromycin in human plasma by high-
311 performance liquid chromatography with spectrophotometric detection. *J Chromatogr B*
312 *Biomed Sci Appl.* 1999; 723(1-2):233-238.
- 313 14. Lim JH, Park BK, Yun HI. Determination of roxithromycin by liquid chromatography/mass
314 spectrometry after multiple-dose oral administration in broilers. *J Vet Sci.* 2003; 4(1):35-
315 40.
- 316 15. FDA Center for Drug Evaluation and Research. Reviewer Guidance: Validation of
317 Chromatographic Methods. 1994. Division of Communications Management, FDA,
318 Rockville, Maryland, USA.
- 319 16. Harris DC. Quality assurance and calibration methods. In: Harris DC, Lucy CA, editors.
320 *Quantitative Chemical Analysis*, 9th ed. New York: W.H. Freeman and Company, 2016;
321 pp. 95-112.
- 322 17. International Conference on Harmonisation. Harmonised Tripartite Guideline Q2(R1).
323 Validation of analytical procedures: text and methodology. International Conference on
324 Harmonisation (ICH) of technical requirements for registration of pharmaceuticals for
325 human use. 2005. Available: <https://www.ich.org/> Accessed on 11th October 2019.
- 326 18. Croteau D, Vallee F, Bergeron MG, LeBel M. High-performance liquid chromatographic
327 assay of erythromycin and its esters using electrochemical detection. *J Chromatogr B*
328 *Biomed Sci Appl.* 1987; 419:205-12.
- 329 19. Pappa-Louisi A, Agrafiotou P. Reversed-phase liquid chromatographic behavior of the
330 macrolide antibiotics clarithromycin and roxithromycin. *Chromatographia.* 2002; 55(9-
331 10):541-7.
- 332 20. Young RA, Gonzalez JP, Sorkin EM. Roxithromycin: A review of its antibacterial activity,
333 pharmacokinetic properties and clinical efficacy. *Drugs.* 1989; 37(1):8-41.
- 334 21. Hannan PC. Guidelines and recommendations for antimicrobial minimum inhibitory
335 concentration (MIC) testing against veterinary mycoplasma species. *Vet Res.* 2000;
336 31(4):373-95.
- 337 22. United States Environmental Protection Agency (2003). Method 8000C: Determinative
338 Chromatographic Separations. SW846, 8000C, Section 11.4.3, Revision 3, 2003. US-
339 EPA, USA.